

Vertical autoclaves with drying

AE-DRY Series CLASSIC LINE

Technical information



Why choose RAYPA?

Expert manufacturer, original design, global brand



GLOBAL REACH

With half a century of experience, we have a long list of satisfied customers around the world. Currently, we export 85% of our annual turnover and have a stable network of distributors with presence in over 100 countries.



EFFICIENT TECHNICAL SERVICE

Our team of highly qualified technicians and engineers is expert in our products. If you experience a technical issue, it will be our priority to rectify it. When you purchase a RAYPA unit, you're guaranteed top-level support and technical assistance.



EXPERT MANUFACTURER

After more than 45 years in the industry, RAYPA is a global leader in the manufacture of laboratory autoclaves. Each of our autoclaves is designed and manufactured entirely within our modern facility equipped with the latest technology.



FULL AND CUSTOMIZABLE RANGE

We offer an extensive portfolio of laboratory autoclaves to cover multiple applications and market segments. Discover the combination of autoclave model and accessories that best fits your needs within our 11 series and 35 available models.



INNOVATION AND QUALITY

Our products feature advanced technology, ongoing innovation, superior construction quality, and are designed for a long service life. Our technical and engineering staff works tirelessly every day to optimize our products and exceed our customers' expectations.



COMPREHENSIVE CONSULTANCY

Our team of specialists assesses each project and provides guidance to clients on the option that best suits their requirements. After the sale, we offer training on the use and recommended maintenance of each unit to ensure its optimal operation and extend its lifespan.

Vertical autoclaves with drying

AE-DRY Series vertical floor-standing autoclaves with top-loading access cover most laboratory sterilization needs in many industries, educational institutions and research facilities with the aim of increasing the productivity of the laboratory. With a spacious chamber, the vacuum drying function and the integrated water tank, along an optimized use of resources like water, energy, and time, these autoclaves provide an efficient and cost-effective solution to handle laboratory workloads effectively.

RECOMMENDED APPLICATIONS

- Culture media and liquids
- Glassware
- Plastics and metal objects
- Laboratory waste bags
- Porous solids and wrapped objects*

*For this application, the sterilization time must be extended, the chamber should not be fully loaded, and chemical and/or biological tests should be used to validate the proper sterilization of the load.



MAIN FEATURES

COST-EFFECTIVE SOLUTION

AE-DRY Series autoclaves are robust and offer excellent performance for liquids and solids sterilization procedures. The final vacuum drying feature by a heating jacket and a vacuum pump at the end of the sterilization cycle eliminates the need of an external equipment to dry the load, significantly reducing the duration of each sterilization procedure rotation and saving operator time.

MULTIPLE TYPES OF STERILIZATION

Several options available to perform sterilization of solids or liquids. Programmable final vacuum drying for the sterilization of solids, initial prevacuum for the sterilization of items of complex geometries and programmable temperature holding at the end of the cycle for the sterilization of culture media. Additionally, an optional flexible temperature probe is available for precise liquid sterilization.

EASY INSTALLATION AND MAINTENANCE

AE-DRY Series autoclaves are plug and play devices, requiring no special installation connections. They operate with just an electrical connection and can function without a drain. Each unit features an integrated water tank that automatically supplies the sterilization chamber, which is manually filled. For added convenience, an optional upgrade allows full automation of water supply directly from a water network. All models are equipped with casters, enabling easy mobility and use in different locations.

SAFETY FIRST

AE-DRY Series autoclaves are designed with several features to ensure the safety of the operators. These include an overpressure safety valve, a thermally insulated door, an overtemperature safety thermostat, a water level sensor,, an open door detection system and an independent safety pneumatic system that locks the main door while positive pressure is present in the sterilization chamber.

ADVANTAGES

!!!	Equipped with heating jacket and vacuum pump to obtain a completely dry load at the end of a solids program.	■	Suitable to sterilize wrapped and unwrapped loads, small porous and hollow objects and items of complex geometries with cavities thanks to the standard initial prevacuum phase.
	The sterilization chamber and door are made of high- quality AISI-316L stainless steel, providing exceptional resistance to corrosion.	0	Automatic water supply from the integrated water tank to the sterilization chamber, with water level sensors at both locations. Optional upgrade for
C€	Autoclaves manufactured in full compliance with all applicable European Union quality, regulatory and safety standards.	l °£	automatic supply from a water network. Adjustable temperature holding at the end of the sterilization cycle between 40-80°C (agar mode).
ß	Steam generation by powerful Incoloy® 825 electric heating elements assembled inside the sterilization chamber and shielded by a protective grid.		Programmable auto-start for up to 24h.
(Control by a PID microprocessor with 4 predefined and 6 editable programs, adjustable by time, temperature,	E)	Plug and play equipment, no plumbing required.
	drying time and type of sterilization cycle (solids or liquids, with optional agar mode and/or flexible temperature probe control).	0	Seamless mobility, all models include casters.
			Optional software for sterilization data management.
4	Available special models with increased heating capacity to achieve faster heating and sterilization phases.	凸	Optional embedded or external printer.

WORKING PRINCIPLE

AE-DRY Series autoclaves provide a solution for the multiple sterilization needs of a general laboratory, including glassware, plastics, metal utensils, laboratory waste bags, wrapped and unwrapped loads, small porous and hollow objects, liquids, culture media, and other laboratory items.

The load has to be placed in baskets inside the chamber, and after manually filling the independent clean water tank with purified water, the equipment starts to create the initial prevacuum, automatically supplies water to the sterilization chamber, heats up and purges until the pre-programmed combination of sterilization time and temperature is reached.



OPERATION OF A STERILIZATION CYCLE FOR SOLID LOADS

PREVACUUM PHASE

- In this initial step, the equipment's vacuum pump mechanically removes air from the chamber and load through a single vacuum pulse of -0,75 Bargs. This allows the steam to penetrate load objects of difficult geometries.
- Afterwards, the independent water tank starts to supply water to the sterilization chamber.

HEATING PHASE

- After completing the prevacuum phase and once the sterilization chamber bottom is filled with water, the powerful heating elements assembled at the bottom of the sterilization chamber heat up dramatically, transferring energy to water to produce saturated steam throughout the chamber.
- To shorten the duration of this step, RAYPA offers special models with increased heating capacity, a feature of particular interest for autoclaves operating in laboratories with high workloads.

STERILIZATION PHASE


- Upon reaching the set sterilization temperature inside the chamber, the sterilization phase begins accurately sustaining the temperature throughout the duration of this phase.
- This crucial step is controlled by a PT-100 Class A temperature probe located within the chamber. As an option for liquids sterilization processes, this phase can be regulated by a flexible PT-100 Class A temperature probe located inside a sample.

VACUUM DRYING PHASE

 Once the sterilization phase is completed, only in solids programs, a vacuum drying phase begins, in which multiple vacuum pulses are produced by means of a vacuum pump and heating jacket to completely dry the load. The water is automatically returned to the integrated water tank.

COOLING PHASE

- Finally, a natural cooling phase begins. A beep will sound when a safe temperature is reached allowing the chamber to be opened.
- In liquid programs with agar mode, the preprogrammed temperature (selectable between 40°C and 80°C) will be maintained indefinitely.

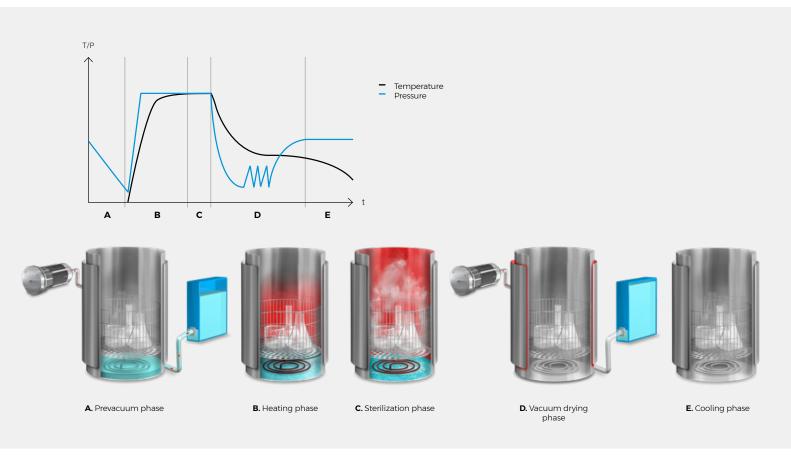

PREDEFINED PROGRAMS

Program N°	Sterilization temperature °C	Sterilization time min	Drying time min	Program mode
P0	115	60	12	Solids
P1	121	30	25	Solids
P2	133	20	30	Solids
P3	121	20	-	Liquids


AE-DRY Series autoclaves have 10 programs, from P0 to P9, and the first four are predefined and protected.

The remaining programs from P4 to P9, can be edited by setting the following parameters:

- · Sterilization temperature.
- · Sterilization time.
- · Final drying time.
- \cdot Sterilization mode (solids or liquids)
- Sterilization with temperature maintenance at the end of the cycle (agar mode).
- Temperature control of the sterilization cycle can be performed by the chamber temperature probe or by the combined use of the chamber probe and the flexible probe.

DIGITAL MICROPROCESSOR

Digital PID microprocessor with 6 push-buttons for simple programming and parameter selection.

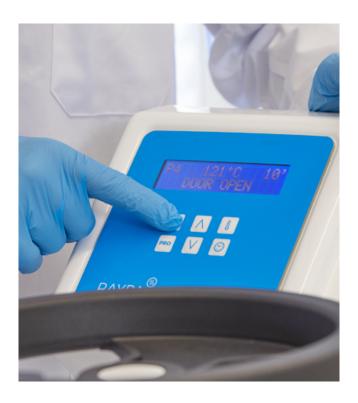

FUNCTIONS OF THE DISPLAY

The alphanumeric screen apart from showing the standard sterilization parameters also shows current sterilization phase and several visual alerts, including warning or failure messages. The available languages include English, Spanish, French and Catalan. To install other languages, please contact us.



LOADING CAPACITIES



ISO ERLENMEYER FLASKS

		250mL (Ø85 x 143mm)			((500mL (Ø105 x 183mm)			1000mL (Ø131 x 230mm)			2000mL (Ø166 x 280mm)					
Autoclave volume baskets basket			Tota	l units	Total baskets	Units / basket	Tota	l units	Total baskets	Units / basket	Total	units	Total baskets	Units / basket	Tota	I units	
	Α	В	A B		A B					Α	В						
AE-28-DRY	31	2	7	14	=	1	4	4	8	1	1	1	=	1	1	1	=
AE-50-DRY	50	3	7	21	28	1	4	4	12	1	1	1	=	1	1	1	2
AE-75-DRY	75	3	12	36	=	2	8	16	24	2	5	10	=	1	3	3	6
AE-110-DRY	110	4	12	48	60	3	8	24	32	3	5	15	=	1	3	3	6
AE-150-DRY	153	4	21	84	105	4	14	56	=	3	8	24	=	1	5	5	10



ISO BOTTLES

		250mL (Ø70 x 143mm)			(500mL (Ø80 x 185mm)			1000mL (Ø101 x 230mm)			2000mL (Ø136 x 260mm)					
Usable Autoclave volume	Total baskets	Units / basket	Total	units	Total baskets	Units / basket	Tota	l units	Total baskets	Units / basket	Total	units	Total baskets	Units / basket	Tota	l units	
model	L			Α	В			Α	В			Α	В			Α	В
AE-28-DRY	31	2	9	18	=	1	7	7	14	1	4	4	=	1	1	1	=
AE-50-DRY	50	3	9	27	36	1	7	7	21	1	4	4	=	1	1	1	2
AE-75-DRY	75	3	20	60	=	2	14	28	42	2	8	16	=	1	4	4	8
AE-110-DRY	110	4	20	80	100	3	14	42	56	3	8	24	=	1	4	4	12
AE-150-DRY	153	4	33	132	165	4	24	96	=	3	15	45	=	1	8	8	16

The data contained within these tables, regarding load capacities, serves as a non-binding guide to assist you in the selection of the most appropriate autoclave model.

A: Number of units using standard baskets.

B: Number of units using specially designed baskets for the specific combination of autoclave model and container.

A: Number of units using standard baskets.

B: Number of units using specially designed baskets for the specific combination of autoclave model and container.

ACCESSORIES

INTEGRATED BASKET LIFT SYSTEM

References		CLASSIC-LIFT	CLASSIC-LIFT-R
Dimensions L x D x H mm		800 x 300 x 2100	800 x 300 x 2600
Power W		480	480
Voltage ∨		230	230
Frequency Hz		50/60	50/60
Weight Kg		40	45
Maximum load Kg		30	40
	79 L	✓	-
For autoclaves with the following chamber volumes	115 L	~	✓
	175 L	-	✓

- $\boldsymbol{\cdot}$ Stainless steel electric lift system built into the side of the autoclave with swivel arm to help load and unload heavy items. Push-button operation with opening up to 200°
- · Motor with auto brake system in the event of obstacles or overload.
- · Available in two models: the standard lift system and reinforced lift system.
- \cdot It can be factory fitted or retrofitted.



MOBILE BASKET LIFT SYSTEM

Reference	MOB-LIFT
Dimensions L x D x H mm	420 x 800 x 2200
Power W	200
Voltage V	115 - 230
Frequency Hz	50/60
Weight Kg	85
Maximum load Kg	30

- $\boldsymbol{\cdot}$ Stainless steel electric lift system with casters to help load and unload heavy items up to 30Kg.
- $\boldsymbol{\cdot}$ Equipped with long-life battery for cordless use.
- · Push-button operation.
- $\boldsymbol{\cdot}$ Motor with auto brake system in the event of obstacles or overload.
- · Compatible with any autoclave model.



ACCESSORIES

STAINLESS STEEL WIRE BASKETS FOR STERILIZING CLEAN LOADS OR HEAVY ITEMS

References		CV-28	CV-75-130	CV-75S	CV-75	CV-150-130	CV-150S	CV-150M
Dimensions	External Ø x H mm	270 x 185	370 x 130	370 x 180	370 x 265	470 x 130	470 x 190	470 x 235
	Internal Ø x H mm	260 x 180	360 x 125	360 x 175	360 x 260	460 x 125	460 x 185	460 x 230
N 4 i	33 L	2	-	-	-	-	-	-
Maximum capacity for	55 L	3	-	-	-	-	-	-
autoclaves with	79 L	-	4	3	2	-	-	-
the following	115 L	-	6	4	3	-	-	-
chamber volumes	175 L	-	-	-	-	6	4	3



STAINLESS STEEL LIQUIDS COLLECTOR TRAY FOR WIRE BASKETS

References		TR-270	TR-370	TR-470
Dimensions	External Ø x H mm	240 x 50	320 x 50	420 x 50
Dimensions	Internal Ø x H mm	238 x 48	318 x 48	418 x 48
	CV-28	✓	-	-
For the following wire baskets models	CV-75S & CV-75	-	~	-
models	CV-150S & CV-150M	-	-	~



UNPERFORATED STAINLESS STEEL BASKETS FOR STERILIZING DIRTY LOADS OR OBJECTS WITH RISK OF SPILLAGE

References		CCI-28	CCI-75S	CCI-75	CCI-150S	CCI-150M
Dimonoiono	External Ø x H mm	270 x 185	370 x 180	370 x 265	470 x 190	470 x 235
Dimensions	Internal Ø x H mm	260 x 180	360 x 175	360 x 260	460 x 185	460 x 230
Massimosm	33 L	2	-	-	-	-
Maximum capacity for	55 L	3	-	-	-	-
autoclaves with	79 L	-	3	2	-	-
the following chamber volumes	115 L	-	4	3	-	-
	175 L	-	-	-	4	3



STAINLESS STEEL "SCHIMMELBUSCH" DRUM FOR STERILIZING INSTRUMENTS AND BIOHAZARDOUS LOADS

References		TBE-24x16	TBE-34x24	TBE-48x24
Dimonoiono	External Ø x H mm	240 x 165	340 x 240	480 x 240
Dimensions	Internal Ø x H mm	230 x 155	330 x 230	470 x 230
	33 L	2	-	-
Maximum capacity for	55 L	4	-	-
autoclaves with the following	79 L	-	2	-
chamber volumes	115 L	-	3	-
	175 L	-	-	3



ACCESSORIES

STAINLESS STEEL CYLINDERS FOR STERILIZING PETRI DISHES

References		CEP-1027	CEP-1041	CEP-1427	CEP-1441
Dimensions	External Ø x H mm	100 x 270	100 x 410	140 x 270	140 x 410
Petri dishes	Maximum number dishes / cylinder	10	18	10	18
	Diameter Ø mm	80	80	120	120
Maniana	33 L	4	4	2	2
Maximum capacity for	55 L	8	4	4	2
autoclaves with	79 L	16	8	10	5
the following chamber volumes	115 L	24	16	15	10
	175 L	28	14	16	8



STAINLESS STEEL CYLINDERS FOR STERILIZING PIPETTES

	CEPP-726	CEPP-740	CEPP-1025	CEPP-1435
External Ø x H mm	70 x 260	70 x 400	100 x 250	140 x 350
Internal Ø x H mm	60 x 250	60 x 390	90 x 240	130 x 340
33 L	11	11	6	6
55 L	22	11	12	12
79 L	42	21	20	10
115 L	63	42	30	20
175 L	90	30	51	34
	Internal Ø x H mm 33 L 55 L 79 L 115 L	External Ø x H mm 70 x 260 Internal Ø x H mm 60 x 250 33 L 11 55 L 22 79 L 42 115 L 63	External Ø x H mm 70 x 260 70 x 400 Internal Ø x H mm 60 x 250 60 x 390 33 L 11 11 55 L 22 11 79 L 42 21 115 L 63 42	External Ø x H mm 70 x 260 70 x 400 100 x 250 Internal Ø x H mm 60 x 250 60 x 390 90 x 240 33 L 11 11 6 55 L 22 11 12 79 L 42 21 20 115 L 63 42 30



STAINLESS STEEL WIRE BASKET WITH HEIGHT ADJUSTABLE TRAYS

References External dimensions Ø x H mm			SRA-R-300	SRA-R-400	SRA-R-500 450 x 180	
			250 x 190	350 x 180		
Trava	Reference	3	TRAY-SRA-R-300	TRAY-SRA-R-400	TRAY-SRA-R-500	
Trays	Dimension	ons Ø x H mm 240 x 20		340 x 20	440 x 20	
		33 L	2	-	-	
Maximum capacity for autoclaves with the following chamber volumes 55 L 79 L 115 L 175 L		3	-	-		
		-	3	-		
		115 L	-	4	-	
		175 L	-	-	4	



- $\cdot \ \text{For sterilization of instruments, small bags and other small objects that must be placed straight up.}\\$
- · Material: AISI-304 stainless steel.



ACCESSORIES



FLEXIBLE TEMPERATURE PROBE PT-100 CLASS A

After installing this accessory, the temperature regulation of the sterilization cycle can either be controlled by the main chamber temperature probe or both the main chamber temperature probe and the flexible temperature probe.

The temperature control by the flexible temperature probe is especially advantageous for processes involving the sterilization of large volumes of liquids, where the sterilization process is regulated by both the temperature achieved in the center of the liquid sample as well as the temperature achieved in the sterilization chamber. Furthermore, should the autoclave be opened at chamber temperatures higher than 80°C there is a risk of liquids boiling over which can be avoided if the temperature of the sample is controlled throughout the sterilization procedure.

Must be installed in our facilities.

Ref. PT-2



Download technical data sheet



EXTERNAL DOT MATRIX PRINTER

Prints program number, cycle number, temperature, pressure, date and hour and error messages.

Selectable print frequency between 10 and 240 seconds.

Connection: RS-232.

Consumables: PAPER-ITS for paper and 70945 for ribbon.



Download technical data sheet



SOFTWARE SW7000

Communication software between the equipment and the PC for display and recording in real time or display after each cycle. Cycles can also be printed or exported to Excel.

PC connection via RS-232.

It is supplied with an RS-232 cable, a USB memory stick including installation software and drivers, and an RS-232 to USB adapter.

Ref. SW7000



EMBEDDED THERMAL PRINTER

rints program number, cycle number, temperature, pressure, date and hour of the run and error messages.

Selectable print frequency between 10 and 240 seconds.

Must be installed at our factory.

Consumable: PAPER-IT for paper



Download technical data sheet



CABLE GLAND

Installation of a Ø2mm or Ø4mm cable gland to provide access to as many as 8 external temperature probes for calibration and validation procedures.

Ref. CG2MM & CG4MM



Download technical data sheet

ACCESSORIES



EXTERNAL TEMPERATURE PROBE ADAPTER

External adapter for continuous validation processes that provides access to an external probe (Ø3-6mm) to take temperature readings that are independent of the equipment microprocessor.

It is located on the autoclave door. Must be installed at our factory.

Ref. EXT-TP



Download technical data sheet



TRANSPORT TROLLEY

Auxiliary trolley to aid in the loading and unloading of the autoclave.

Made of chrome iron and plastic.

The surface of each shelf is textured to prevent the load from moving.

Equipped with rubber casters to reduce noise and prevent floor wear.

Dimensions (LxDxH): 730x490x700mm

Ref. TR-TR



Download technical data sheet



PREMIUM CASTERS

Although all AE-DRY Series autoclaves include casters, this accessory offers the option of upgrading to stronger, medical grade casters that include brakes.

This enhances the mobility of the equipment.

Must be installed at our factory.

Ref: 4WHBR



ECO-EFFICIENT WATER PURIFIER

Eco-efficient direct-flow water purifier with LED display and no accumulation of water. Capable of filtering 1,3L/min.

The installation of this accessory requires the joint installation of the external tank (TANK-KLL) and the automatic water filling system (KLL).

Ref. ECOPUR-500



Download technical data sheet



PURIFIED WATER TANK

Alternative solution for the storage of up to 25L of purified water in the absence of a water network.

Ref. TANK-KLL



Download technical data sheet



AUTOMATIC WATER FILLING KIT

Water pump for automating the supply of purified water to the integrated water tank.

Compatible with installations with a purified water network or a purified water tank, or installations with a non purified water network; in the latter case, a water purifier (ECOPUR-500) and a purified water tank (TANK-KLL) will be required.

Must be installed at our factory.

Ref. KLL



Download technical data sheet

ACCESSORIES



TEMPERATURE DATA LOGGER

AISI-316L stainless steel disk temperature recorder with connection base and software.

Recommended for autoclave validation and for monitoring the internal temperature of containers.

Available in different sizes.

Ref. BDL-DISK3618_CL



Download technical data sheet



STERILIZATION CONTROL TAPE

Class 1 indicator for steam sterilization. The color change indicates that the materials have been processed; however, this does not guarantee adequate sterilization. Additional methods, such as biological indicators (EN ISO 11138), are required.

Pack of 5 rolls of 50m x 19mm tape.

Ref. TEST-CT



J Download technical data sheet

SPECIFIC SERVICES



IQ-OQ DOCUMENTATION

Delivery of documentation and protocols for autoclave qualification through a third party.

Ref. IQ-OQ DOC

Download technical data sheet



IQ-OQ-PQ QUALIFICATION

Autoclave qualification service performed by RAYPA technicians or authorized entities. It covers the startup of the equipment and the comprehensive qualification of its performance.

Ref. IQ-OQ-PQ

Download technical data sheet



CALIBRATION CERTIFICATE FOLLOWING ENAC TRACEABILITY STANDARDS

Unitary certification of proper equipment calibration and performance in compliance with international standards.

Ref. MAPEO-ENAC



MAPPING OF STABILITY AND **HOMOGENEITY**

Generation of documentary evidence certifying that the temperature and pressure distribution within the autoclave is uniform and stable, in accordance with the manufacturer's design specifications.

Ref. MAP-3, MAP-7 and MAP-9



ON-SITE COMMISSIONING & TRAINING

On-site commissioning, which includes verification of the correct operation and installation of the equipment and a training session for users on the use and maintenance of the equipment.

Ref. INSAE

Download technical data sheet



REMOTE COMMISSIONING & TRAINING

Guided remote startup including a training session for users on the operation and maintenance of the equipment.

Ref. INSAE-REM



Download technical data sheet



MAINTENANCE CONTRACT

Regular inspection plan that includes technical inspection, probe calibration and compliance with the preventive maintenance plan, in addition to tariff

Ref. MANT-1.2 and MANT-1.3



EXTENDED WARRANTY

Extended warranty up to a total of 3 vears


Ref. WE-CL



SET OF CONSUMABLES, **SPARE PARTS AND ESSENTIAL COMPONENTS**

Set of original spare parts, consumables and components, chosen specifically to adhere to each model's maintenance plan, intended to maximize equipment longevity and minimize downtime in the event of a malfunction.

TECHNICAL DRAWINGS OF THE AUTOCLAVE

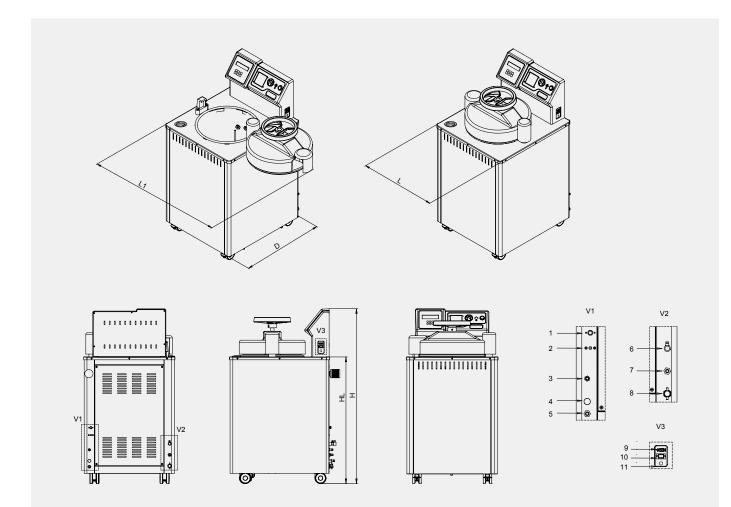


MODELS	L LENGTH with closed door	L1 LENGTH with maximum door opening	D DEPTH	H HEIGHT	HL LOAD HEIGHT
AE-28-DRY	505 mm	900 mm	580 mm	1110 mm	788 mm
AE-50-DRY	505 mm	900 mm	580 mm	1290 mm	967 mm
AE-75-DRY	610 mm	1100 mm	700 mm	1185 mm	862 mm
AE-110-DRY	610 mm	1100 mm	700 mm	1435 mm	1112 mm
AE-150-DRY	750 mm	1380 mm	820 mm	1400 mm	1073 mm

CONNECTIONS

1	Sterilization chamber electrical heating elements safety thermostat
2	Heating jacket safety thermostat
3	Power supply cable (AE-110-DRY and AE-150-DRY models)
4	Safety valve outlet
5	Automatic water supply inlet
6	Independent clean water tank drain outlet

7	Independent clean water tank overflow outlet		
8	Access to the drain filter and sterilization chamber drain outlet		
9	RS-232 Port		
10	Ethernet Port		
11	Power supply cable (AE-28-DRY, AE-50-DRY y AE-75-DRY models)		

TECHNICAL DRAWINGS OF THE AUTOCLAVE + CLASSIC-LIFT

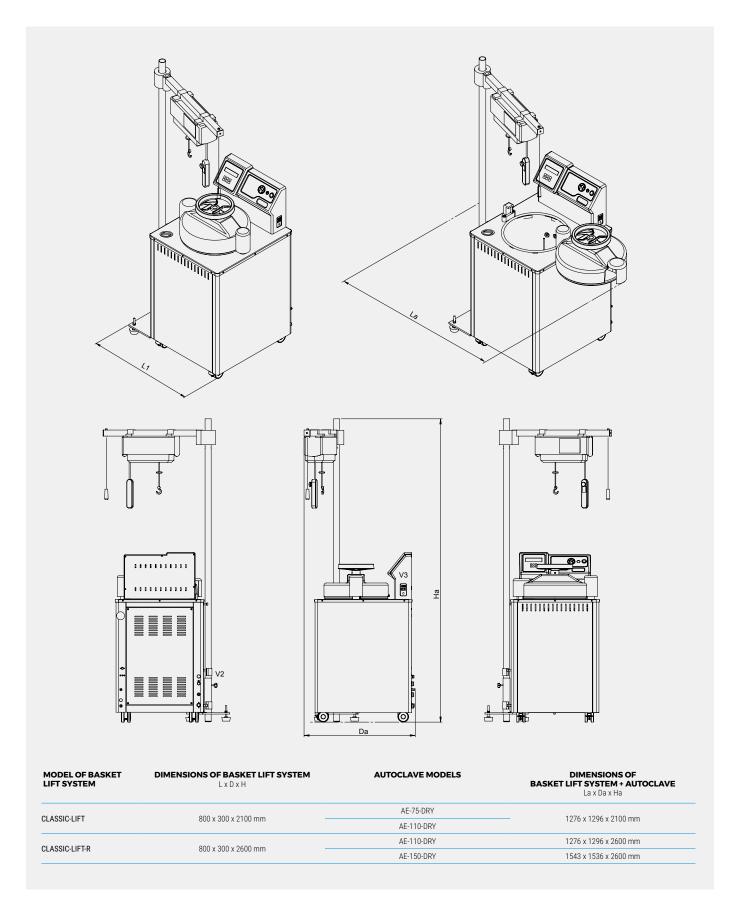

TECHNICAL SUMMARY

		Recommended setting	General laboratory
\Diamond		Equipment placement	Floor-standing
493	General classification	Load direction	Top-loading
		Chamber profile	Round
	Recommended type of load Sterilization technology	Glassware	++
П		Culture media and liquids	++
<u>///</u>		Laboratory waste bags	++
		Porous solids and wrapped loads	+
		Method to generate steam	Heating elements
(1/1)		Type of purge	Vacuum
		Vacuum drying by heating jacket and vacuum pump	✓
·1)))	Transfer of data	RS-232	~
	Datab asinta	Embedded printer	0
ایت	Batch printers	External printer	0
		Sterilization chamber volume	33 - 175 L
		External building material	AISI-304
		Sterilization chamber material	AISI-316L
		Heating elements material	Incoloy® 825
		Gasket material	Silicone rubber
8	Sterilization chamber and door specifications	Min max. sterilization temperature	100 - 134 °C
		Maximum pressure (above atmospheric pressure)	2,1 Barg
		Mechanism to open the door	Manual wheel
		Direction in which the door opens	Lateral
		Automatic locking with pressure	✓
		Thermally insulated door	✓
	User interface and microprocessor	Screen display	Digital LCD
		Screen size	2 lines x 16 digits
		Total number of available programs	
	User interface and microprocessor	rotal nambol of aranapic programs	10
	User interface and microprocessor	Automatic microprocessor control	10 ✓
	User interface and microprocessor		
<u>.</u>	User interface and microprocessor	Automatic microprocessor control	~
	User interface and microprocessor Special cycles and process optimization	Automatic microprocessor control Timer start	∀
		Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C)	
		Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads)	* * * *
		Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe	* * * * * 0
	Special cycles and process optimization	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode	• • • • • • • • • • • • • • • • • • •
`\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\		Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature	• • • • • • • • • • • • • • • • • • •
	Special cycles and process optimization	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase	• • • • • • • • • • • • • • • • • • •
	Special cycles and process optimization	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase	• • • • • • • • • • • • • • • • • • •
` <u>`</u>	Special cycles and process optimization	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase Temperature regulation by flexible probe	• • • • • • • • • • • • • • • • • • •
` <u>`</u>	Special cycles and process optimization	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase Temperature regulation by flexible probe Sterilization mode (solids or liquids)	• • • • • • • • • • • • • • • • • • •
`\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\	Special cycles and process optimization	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase Temperature regulation by flexible probe Sterilization mode (solids or liquids) Air intake with bacteriological filter	40 - 80 °C 100 - 134 °C 1 - 250 min 3 - 99 min On/Off
`\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\	Special cycles and process optimization Adjustable cycle parameters	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase Temperature regulation by flexible probe Sterilization mode (solids or liquids) Air intake with bacteriological filter Independent water tank capacity	40 - 80 °C 100 - 134 °C 1 - 250 min 3 - 99 min On/Off 9 - 20 L
`\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\	Special cycles and process optimization	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase Temperature regulation by flexible probe Sterilization mode (solids or liquids) Air intake with bacteriological filter Independent water tank capacity Flexible temperature probe	0 40 - 80 °C 100 - 134 °C 1 - 250 min 3 - 99 min On/Off 4 9 - 20 L 0
`\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\	Special cycles and process optimization Adjustable cycle parameters	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase Temperature regulation by flexible probe Sterilization mode (solids or liquids) Air intake with bacteriological filter Independent water tank capacity Flexible temperature probe Standard casters	40 - 80 °C 100 - 134 °C 1 - 250 min 3 - 99 min On/Off 9 - 20 L 0
`\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\	Special cycles and process optimization Adjustable cycle parameters	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase Temperature regulation by flexible probe Sterilization mode (solids or liquids) Air intake with bacteriological filter Independent water tank capacity Flexible temperature probe Standard casters Premium casters with brakes	0 40 - 80 °C 100 - 134 °C 1 - 250 min 3 - 99 min On/Off 4 9 - 20 L 0
`\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\	Special cycles and process optimization Adjustable cycle parameters	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase Temperature regulation by flexible probe Sterilization mode (solids or liquids) Air intake with bacteriological filter Independent water tank capacity Flexible temperature probe Standard casters Premium casters with brakes Pressure gauge Electric customization (115-230M V / 230-400T V)	• • • • • • • • • • • • • • • • • • •
`;	Special cycles and process optimization Adjustable cycle parameters	Automatic microprocessor control Timer start Agar mode (temperature holding after cycle ends 40-80°C) Final postvacuum drying (to completely dry solid loads) Temperature regulation by flexible probe Agar mode Sterilization phase temperature Duration of sterilization phase Duration of drying phase Temperature regulation by flexible probe Sterilization mode (solids or liquids) Air intake with bacteriological filter Independent water tank capacity Flexible temperature probe Standard casters Premium casters with brakes Pressure gauge	• • • • • • • • • • • • • • • • • • •

^{+:} Recommended ✓: Standard 0: Optional

TECHNICAL DATA











Specifications

Specifications					
References	AE-28-DRY	AE-50-DRY	AE-75-DRY	AE-110-DRY	AE-150-DRY
Total/usable volume of the chamber L	33/31	55/50	79/75	115/110	175/153
Usable dimensions of the chamber Ø x H mm	300 x 440	300 x 710	400 x 600	400 x 850	500 x 760
External dimensions L x D x H mm	505 x 580 x 1110	505 x 580 x 1290	610 x 700 x 1185	610 x 700 x 1435	750 x 820 x 1400
Loading height mm	795	975	870	1120	1085
Net weight Kg	75	95	123	150	235
Available heating capacities W	2000 or 2800	2800 or 5000	3200 or 6000	4500, 6000 or 9000	6000 or 9000
Standard voltage* V	230	230	230	400	400
Frequency Hz	50/60	50/60	50/60	50/60	50/60

^{*}Other voltages and electrical configurations available on request. Special models with increased heating capacity may operate with other voltages.

Safety features

- · Safety valve.
- Safety thermostats with manual rearm for the heating jacket and the heating elements.
- Pneumatic door blocking system while positive pressure exists inside the sterilization chamber.
- Open door sensor.
- Thermally insulated door.
- · Water level detector in the sterilization chamber.
- Water level detector (min./max.) in the independent water tank.
- Bacteriological filter for inlet air.
- Heating elements cover.Several visual and acoustic safety and warning alarms.

Regulations

All our AE-DRY Series autoclaves are designed to comply with the strictest international directives and standards, including the following

- EN-61010-1 Safety requirements for electrical equipment for measurement, control and laboratory use. Part 1: General requirements.
- EN-61010-2-040 Part 2-040: Requirements for laboratory autoclaves.
- EN-61326 Electrical equipment for measurement, control and laboratory use. EMC requirements.
 AD 2000 Merkblatt Pressure vessels.
- · 2014/35/UE Low voltage.
- · 2014/30/UE Electromagnetic compatibility.
- · 2014/68/UE Pressure equipment.

Comoral footures

General features	
Adjustable sterilization temperature	100 - 134 °C
Adjustable sterilization time	1 - 250 min
Adjustable drying time	3 - 99 min
Max. pressure	2,1 Barg
Sterilization control system	Fully automatic microprocessor control by either chamber temperature probe or flexible temperature probe $ \\$
Air purge system	Mechanical displacement by vacuum pump
Vacuum drying system	Vacuum pump plus heating jacket
External building material	AISI-304 stainless steel
Sterilization chamber material	AISI-316L stainless steel
Heating elements material	Incoloy®825
Gasket material	Silicone rubber
Connection to PC	RS-232
Connection to printer	RS-232 or embedded
Number of programs	10 (4 preset and 6 user free)
Programmable auto-start	Up to 24h
Screen type	LCD display
Opening door mode	Horizontal swiveling door with blocking wheel
Monitoring of sterilization parameters	Self-control of obtained values (To & t) vs programmed values. Cycle is automatically interrupted if obtained values differ from programmed values
Pressure display	Pressure gauge on control panel
Water management	Independent manually fed water tank that automatically supplies the sterilization chamber. Water returns automatically to the independent water tank after completing the sterilization phase. Optional upgrade for full automation of water supply directly from a water network
Drainage system	A drainage connection and a manual valve for overflow and drainage of the independent water tank and a screw to manually clean the drainage filter and drain the sterilization chamber
Casters	Included standard casters. Optional upgrade to medical grade casters with brakes

MORE INFORMATION





◆ Download the installation guide











